

INSTRUCTION MANUAL

No.177SA

Kitagawa WATER VAPOUR DETECTOR TUBES

- ★ READ CAREFULLY THIS INSTRUCTION MANUAL AND THE INSTRUCTIONS OF THE ASPIRATING PUMP PRIOR TO USING THIS PRODUCT.
- ★ DON'T DISCARD THIS INSTRUCTION MANUAL UNTIL ALL THE TUBES IN THIS BOX ARE USED UP.

1. PERFORMANCE:

Measuring Range	1.7 - 33.8 mg/ℓ [From 10% (20 °C=68°F) to 100% (32-90°F)]
and Sampling Time:	20 seconds (1 pump stroke)
Colour Change:	Greenish yellow → Purple
Detectable Limit:	0.2 mg/ℓ
Operating temperature:	0 - 40 °C (32-104°F) (Temperature correction is necessary.)
Aspirating Pump:	Model AP-20, AP-20S, AP-1, AP-1S, 400A or 400B

CAUTION

1. DETECTOR TUBE CONTAINS REAGENTS.
2. DON'T TOUCH THESE REAGENTS DIRECTLY ONCE TUBES ARE BROKEN.
3. KEEP THE TUBES OUT OF THE REACH OF CHILDREN.

NOTICE

1. USE ONLY WITH PUMP MODELS AP-20, AP-20S, AP-1, AP-1S, 400A OR 400B. OTHERWISE, CONSIDERABLE ERROR IN INDICATION MAY OCCUR.
2. DON'T USE FLOW CONTROL ORIFICE WITH THIS TUBE. (FOR MORE DETAIL, REFER TO THE INSTRUCTIONS OF THE ASPIRATING PUMP.)
3. BEFORE TESTING, CHECK THE ASPIRATING PUMP FOR LEAKS (REF. ITEM 7). ANY PUMPS SHOWING SIGNS OF LEAKAGE SHOULD BE CORRECTED BEFORE USE.
4. DON'T USE THIS TUBE OUTSIDE THE STATED OPERATING TEMPERATURE RANGE.
5. STORE TUBES IN A COOL AND DARK PLACE (0-25 °C/32-77°F), AND USE BEFORE EXPIRATION DATE PRINTED ON TOP OF THE BOX.
6. PRIOR TO USE, READ CAREFULLY ITEM 8 "USER RESPONSIBILITY".

2. SAMPLING AND MEASUREMENT:

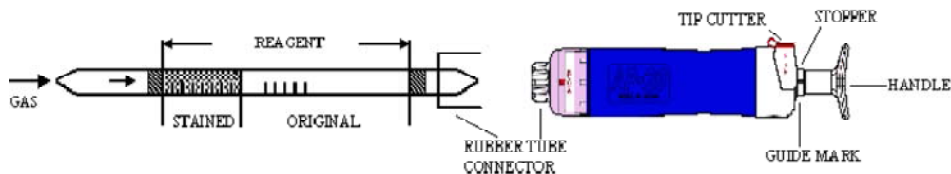


Fig.1

- ① Break both ends of detector tube.

CAUTION SAFETY GLASSES AND GLOVES SHOULD BE WORN TO PREVENT INJURY FROM SPLINTERING GLASS.

- ② Insert the detector tube into aspirating pump securely as shown in Fig.1. (Arrow mark shall point to the pump.)
- ③ Align the guide marks on the shaft and stopper of the aspirating pump.
- ④ Pull the pump handle at full stroke until it locks and wait for 20 seconds or until the completion of sampling is confirmed with the flow indicator of the pump (See descriptions about the flow indicator in the instructions of the pump).
- ⑤ On completion of sampling, read the scale at the maximum point of the stained layer.

SPECIAL NOTE: I. The scale is calibrated at 20 °C (68°F) and 1013hPa. Readings obtained in other circumstances should be corrected (REF. ITEM 3).

II. When the maximum point of the stained layer is unclear, read the scale at the centre between the longest and shortest points.

3. CORRECTION FOR AMBIENT CONDITIONS:

- ① Temperature; Readings from the scale should be corrected with the temperature correction table. The upper temperature correction value indicates relative humidity (%) and the lower value indicates absolute humidity (mg/l).
- ② Atmospheric Pressure;

$$\text{True concentration} = \frac{\text{Temperature corrected concentration} \times 1013}{\text{Atmospheric pressure (in hPa)}}$$


Temperature Correction Table

Scale Readings	0°C 32°F	5°C 41°F	10°C 50°F	12°C 54°F	14°C 57°F	16°C 61°F	18°C 64°F	20°C 68°F	22°C 72°F	24°C 75°F	26°C 79°F	28°C 82°F	30°C 86°F	32°C 90°F	34°C 93°F	36°C 97°F	38°C 100°F	40°C 104°F		
0	100 4.8	50 3.4	30 2.8	20 2.1	18 2.2	15 2.0	12 1.8	10 1.7	9 1.7	8 1.7	7.5 1.8	7 1.9	6.5 2.0	6 2.0	5.5 2.1	5 2.1	4.5 2.3	4 2.0		
5		100 6.8	50 4.7	30 3.2	26 3.1	20 2.7	18 2.8	15 2.5	12 2.3	9 2.0	8 2.0	7.5 2.2	7 2.3	6.5 2.4	6 2.4	5.5 2.5	5 2.5	4.5 2.6	4 2.6	
10			100 9.4	50 7.5	30 5.8	26 4.8	20 4.3	18 4.2	15 3.5	12 3.3	9 3.2	8 3.2	7.5 3.2	7 3.2	6.5 3.0	6 3.1	5.5 3.1	5 3.2	4.5 3.3	
12				100 10.7	50 9.6	30 8.6	26 8.8	20 8.5	18 8.7	15 8.7	12 8.7	9 8.7	8 8.7	7.5 8.7	7 8.7	6.5 8.7	6 8.7	5.5 8.7	5 8.7	
14					100 12.0	50 10.9	30 10.9	26 10.9	20 10.9	18 10.9	15 10.9	12 10.9	9 10.9	8 10.9	7.5 10.9	7 10.9	6.5 10.9	6 10.9	5.5 10.9	5 10.9
16						100 13.6	50 12.3	30 12.3	26 12.3	20 12.3	18 12.3	15 12.3	12 12.3	9 12.3	8 12.3	7.5 12.3	7 12.3	6.5 12.3	6 12.3	5.5 12.3
18							100 15.4	50 13.8	30 13.8	26 13.8	20 13.8	18 13.8	15 13.8	12 13.8	9 13.8	8 13.8	7.5 13.8	7 13.8	6.5 13.8	6 13.8
20								100 17.2	50 15.5	30 15.5	26 15.5	20 15.5	18 15.5	15 15.5	12 15.5	9 15.5	8 15.5	7.5 15.5	7 15.5	6.5 15.5
22									100 19.4	50 17.4	30 17.4	26 17.4	20 17.4	18 17.4	15 17.4	12 17.4	9 17.4	8 17.4	7.5 17.4	7 17.4
24										100 21.8	50 19.5	30 19.5	26 19.5	20 19.5	18 19.5	15 19.5	12 19.5	9 19.5	8 19.5	7.5 19.5
26											100 24.4	50 21.8	30 21.8	26 21.8	20 21.8	18 21.8	15 21.8	12 21.8	9 21.8	8 21.8
28												100 27.2	50 24.2	30 24.2	26 24.2	20 24.2	18 24.2	15 24.2	12 24.2	9 24.2
30													100 30.3	50 27.0	30 27.0	26 27.0	20 27.0	18 27.0	15 27.0	12 27.0
32														100 33.8	50 30.1	30 30.1	26 30.1	20 30.1	18 30.1	15 30.1

4. INTERFERENCES:

Coexistence of more than 0.3% of Methanol, Ethanol, Ethyl acetate or more than 0.5% of Acetone with water vapor respectively produce unclear stains. Coexistence of more than 0.02% of Ammonia with water vapor produces purple and purplish red stains and will give higher readings. Coexistence of more than 0.2% of Nitrogen dioxide with water vapor produces unclear stains.

5. CHEMICAL REACTION IN THE DETECTOR TUBE:



6. DISPOSAL OF TUBE:

USED TUBES SHOULD BE DISCARDED CAREFULLY ACCORDING TO REGULATIONS, IF ANY.

7. INSPECTION OF ASPIRATING PUMP:

Checking for leaks;

- ① Insert sealed, unbroken detector tube into the pump.
- ② Align the guide marks on the shaft and stopper of the pump.
- ③ Pull the handle to full stroke and wait for 3 minutes.
- ④ Unlock the handle and allow it to return slowly into the pump by holding the cylinder and handle securely.

CAUTION HANDLE WILL TEND TO SNAP BACK INTO THE PUMP QUICKLY.

- ⑤ If the handle returns completely to the original position, the performance is satisfactory. Otherwise, refer to maintenance procedure in the pump instructions to correct the fault.

8. USER RESPONSIBILITY:

It is the sole responsibility of the user of this equipment to ensure that the equipment is operated, maintained, and repaired in strict accordance with these instructions and the instructions provided with each Model AP-20, AP-20S, AP-1, AP-1S, 400A or 400B aspirating pump, and that detector tubes are not used which are either beyond their expiration date or have a colour change different to that stated in the Performance specifications.

The Manufacturer and Manufacturer's Distributor shall not be otherwise liable for any incorrect measurement or any damages, whether damages result from negligence or otherwise.

Printed in Japan

IME1770/1